

TABLE OF CONTENTS

	Page
ACKNOWLEDGEMENTS	iii
ABSTRACT (ENGLISH)	iv
ABSTRACT (THAI)	vi
TABLE OF CONTENTS	viii
LIST OF TABLES	xii
LIST OF ILLUSTRATIONS	xiv
ABBREVIATIONS AND SYMBOLS	xviii
CHAPTER 1: INTRODUCTION	
1.1 Calcium, magnesium, iron, zinc and ethanol	1
1.1.1 Importance for determination of calcium, magnesium, iron, zinc and ethanol	1
1.1.2 Methods for determination of calcium, magnesium, iron, zinc and ethanol	5
1.1.2.1 Complexometry of calcium, magnesium, iron, zinc	16
1.1.2.2 On-line derivatization of ethanol	20
1.1.3 Reasons for method development for determinations of calcium, magnesium, iron, zinc and ethanol	21
1.2 Flow Injection Analysis	21
1.3 Detection system	23
1.3.1 Voltammetric detection of derivatized ethanol	23

1.4	Research Aims	24
CHAPTER 2: EXPERIMENTAL		25
2.1	Apparatus and instruments	25
2.2	Chemicals	26
2.3	Preparation of standard solutions and reagents	27
2.3.1	Standard solutions and reagents for the determination of calcium, magnesium, iron and zinc by flow injection colorimetry	27
2.3.2	Standard solution and reagents for on-line derivatization of ethanol prior to voltammetric detection	29
2.4	Studies on FI-colorimetric determination	29
2.4.1	Absorption spectra	29
2.4.2	Manifold for flow injection colorimetry for the determination of calcium, magnesium, iron and zinc	30
2.4.3	Optimization	31
2.5	FI-voltammetric system with on-line derivatization for determination of ethanol	31
CHAPTER 3: RESULTS AND DISCUSSION		34
3.1	FI-colorimetric determination of Ca(II), Mg(II), Fe(II) and Zn(II)	34
3.1.1	Preliminary studies	34
3.1.1.1	Absorption spectra of Mg-EBT complex	34
3.1.1.2	Study of stability of Mg-EBT complex	36
3.1.1.3	Batchwise colorimetric determination of zinc using Mg-EDTA and EBT	38

3.1.1.4 Design and test of FIA system	40
3.1.2 Optimization	42
3.1.2.1 The Mg-EDTA solution	42
3.1.2.2 Effect of EBT concentration	44
3.1.2.3 Effect of mixing coil	45
3.1.2.4 Effect of flow rate	46
3.1.2.5 Effect of pH of standard solution	48
3.1.2.6 Summary of the optimum condition	51
3.1.2.7 Calibration graph and detection limit	51
3.1.2.8 Precision	52
3.1.2.9 Applications	54
3.2 Development of FI-voltammetry and on-line derivatization for determination of ethanol	60
3.2.1 Preliminary studies	60
3.2.1.1 Investigation the reaction behaviour of batchwise system	60
3.2.1.2 Study of OSWV parameters	64
3.2.1.3 Design and construction laboratory made HMDE flow cell	67
3.2.1.4 Test the developed flow cell by analyzing zinc analyte model	68
3.2.2 On-line derivatization combine with HMDE flow cell	69
3.2.2.1 Set up system	70
3.2.2.2 Effect of delay of starting time	71
3.2.2.3 Calibration graph	73

3.2.2.4 Precision	73
3.2.3 Suggestion for FI- on-line derivatization voltammetry for determination of ethanol	74
CHAPTER 4: CONCLUSIONS	75
REFERENCES	77
APPENDICES	84
APPENDIX A Complexation and titration e-book	85
APPENDIX B Voltammetry e-book	86
CURRICURUM VITAE	87

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่
 Copyright © by Chiang Mai University
 All rights reserved

LIST OF TABLES

Table		Page
1.1	Summary of analytical methods for the determination for the determination of calcium, magnesium, iron and zinc using complexing agent	7
1.2	Summary of analytical methods for the determination of ethanol	14
1.3	Formation constants for metal-EDTA complexes	17
1.4	Some of mettalochromic indicators for calcium, magnesium, iron and zinc	18
3.1	Absorbance (530 nm) values of Mg-EBT (replacement of Zn(II) with Mg(II)-EDTA complex) measured in various periods after mixing	37
3.2	Absorbance (530nm) of solutions containing Zn(II) and a mixture of Mg-EDTA (0.05 M) EBT (0.012 % w/v) in NH ₃ /NH ₄ Cl /NH ₄ Cl (0.1 M, pH 10) buffer (measured at 5 min after mixing)	39
3.3	Preliminary conditions for the first set of experiments employing a double line FI manifold (Figure 2.1)	41
3.4	Variation of EDTA in the Mg-EDTA solutions	42
3.5	Effect of mixing coil length on peak height of a series standard Ca(II) solution	45

Table	Page
3.6 Correlation of peak heights and Ca(II) concentrations at various flow rates	47
3.7 Results determined by employing calibration graphs of standards of pH 2	49
3.8 The optimum conditions of the FI-colorimetry procedure for the determination of Ca(II), Mg(II), Fe(II) and Zn(II)	51
3.9 Calibration results for the determination Ca(II), Mg(II), Fe(II) and Zn(II)	52
3.10 Precision studies	53
3.11 The determination results of Ca(II), Mg(II), Fe(II) and Zn(II) in drug and minerals supplements by FI-colorimetry and titrimetry	58
3.12 Precision of overall procedure for determination of Ca(II), Mg(II), Fe(II) and Zn(II)	59
3.13 OSWV conditions for batchwise analysis	61
3.14 Adjustment parameters of OSWV	65
3.15 Size of data file from using various measuring cycle	67
3.16 Starting time (t1) and waiting time (t2)	71
3.17 RSDs (%) for the determination of ethanol by FI- on-line derivatization voltammetry	73


LIST OF ILLUSTRATIONS

Figure	Page
1.1 Structure of EDTA and sodium 1- (1-hydroxy-2-naphthylazo) -6-nitro-2-naphthol-4-sulphonate (II) or Eriochrome Black T (EBT)	18
1.2 A simple flow injection manifold is consisted of pump, injection valve, mixing coil, detector and recorder.	22
2.1 Flow injection system for the determination of calcium(II), magnesium(II), iron(II) and zinc(II); R1= Mg-EDTA reagent in NH ₃ /NH ₄ Cl buffer solution, R2 = EBT reagent in NH ₃ /NH ₄ Cl buffer solution, P = peristaltic, pump, S = injection valve, M = mixing coil, D = colorimeter, R = recorder, and W = waste	30
2.2 Schematic diagram of the FIA manifold for on-line derivatization and detection of ethanol; R1 = supporting electrolyte (0.15 M NH ₄ Cl, 0.03 M NaOH, 0.05 M KH ₂ PO ₄ and 3 x 10 ⁻⁴ M eosin), R2 = 0.1 M NaOH, M = mixing coil, G = gas diffusion unit, V= voltammogram and W = waste	32
2.3 A side view of laboratory-made hanging mercury dropping electrode flow cell	33
3.1 Absorption spectra of solutions recorded against deionized water as reference. (a) 0.0012% w/v EBT + 0.05 M Mg-EDTA + 0.1 M NH ₃ /NH ₄ Cl buffer (blue solution) (b) 2.25 x10 ⁻³ M Zn(II) + 0.0012% w/v EBT + 0.05 M Mg-EDTA + 0.1 M NH ₃ /NH ₄ Cl buffer (wine red solution)	35

Figure	Page
3.2 The absorbance of Zn(II) 0-2.25 mM in 0.0012 % w/v EBT + 0.05 M Mg-EDTA + 0.1 M NH ₃ /NH ₄ Cl buffer pH 10 in various time (0, 30, 150 and 300 min)	37
3.3 Correlation of absorbance and Zn(II) concentration: Mg-EDTA (0.05 M) and EBT(0.012 % w/v) in NH ₃ /NH ₄ Cl (0.1 M, pH 10) buffer	39
3.4 Plots of absorbance (530 nm) vs. metal ion concentration	41
3.5 Study on variation of EDTA concentration by fixing Mg(II) at 8.0 mM for Mg-EDTA reagent for (a) Ca(II), (b) Mg(II), (c) Fe(II) and Zn(II)	43
3.6 FI-grams of Ca(II) obtained	44
3.7 Effect of mixing coil length on peak height of a series standard Ca(II) solution.	46
3.8 Effect of flow rate on peak height (Conditions: A, B, C, D and E) (see Table 3.6)	47
3.9 FI-gram of Ca(II) 4.0 mM under the condition set D	48
3.10 Results of the determination of cations in various pHs (2, 3 and 5) determined by using calibrations graphs prepared by standard solutions of pH 2	49

Figure	Page
3.11 Absorption spectra of Fe(II) (a) 5.0×10^{-4} M (b) 5.0×10^{-3} M (c) 5.0×10^{-2} M in 0.1 M $\text{NH}_3/\text{NH}_4\text{Cl}$ buffer	50
3.12 Osteryoung Square Wave voltammogram of ethyl dithiocarbonate from ethanol 5.0-60 % v/v	62
3.13 Effect of NaOH vs. peak current	63
3.14 Effect of CS_2 volume	64
3.15 Potential waveform for OSWV	64
3.16 Voltammograms of derivatized ethanol 15% v/v at various potential amplitude (U. amp) 5-45 mV (Modul. freq = 50 Hz, U. step = 12 mV and Sweep rate 80 mV/s) (see Table 3.13)	65
3.17 Voltammograms of derivatized ethanol 15% v/v at various potential step (U. step) 4, 6 and 12 mV (Modul. freq = 50 Hz, U. amp=20 mV and Sweep rate 80 mV/s) (see Table 3.13)	66
3.18 Voltammograms of derivatized ethanol 15% v/v at various Modul. freq = 50, 100 and 150 Hz (U. amp = 45 mV , U. step = 12 mV and Sweep rate 80 mV/s) (see Table 3.13)	66
3.19 A manifold and of Zn(II) determination using a laboratory made HMDE flow cell and a time diagram of one injection when t_1 =waiting time1 (injected zone move to flow cell), t_m = measured time (press start button for operate 693 VA processor) and t_2 =waiting time 2 (time for signal down to baseline)	68
3.20 Calibration graph of Zn(II) 0.1-4.0 ppm using FI-voltammetry with a laboratory made flow cell	69


Figure		Page
3.21	Gas-diffusion unit for carbon disulfide using in on-line derivatization system	70
3.22	Plots of delayed starting time vs. peak current of derivatized ethanol 25% v/v from on-line system using equal flow rate of (a) 0.6 mL/min (b) 1.1 mL/min and (c) 2.0 mL/min	71
3.23	Calibration graph	73

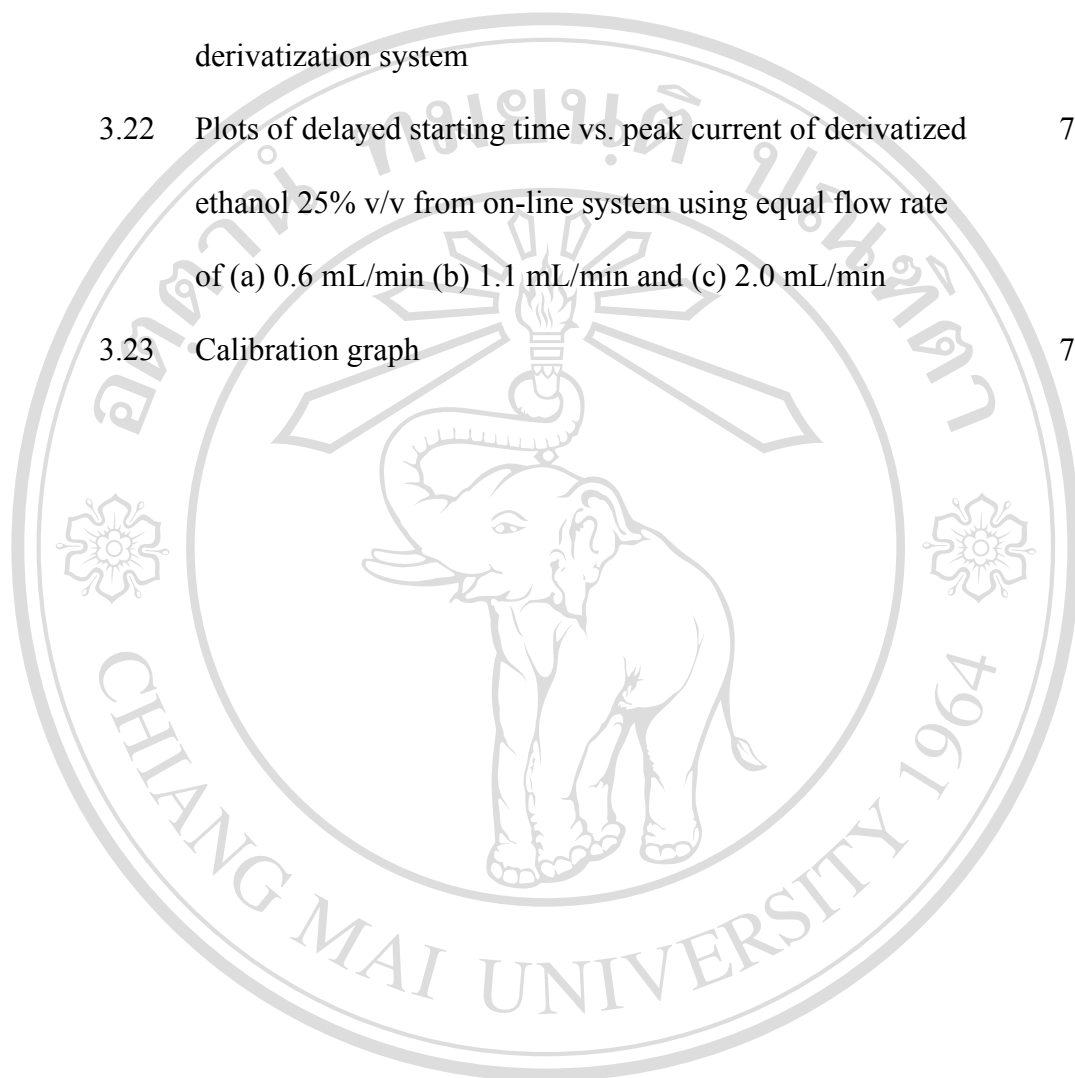

ABBREVIATIONS AND SYMBOLS

AAS	Atomic absorption spectrometry
Abs	Absorbance
ADH	Alcohol dehydrogenase
AOH	Alcohol oxidase
A.E.	Auxiliary electrode
EDTA	Ethylenediaminetetraacetic acid
EGTA	Ethylene glycol-bis (2-aminoethylether) tetraacetic acid
FAAS	Flame atomic absorption spectrometry
FI	Flow injection
FID	Flame ionisation detector
HMDE	Hanging mercury dropping electrode
HPLC	High-performance liquid chromatography
HSGC	Headspace gas chromatography
ICP	Inductively coupled plasma
IEC-EC	Ion-exclusion chromatography- electrochemical detection
LOD	Limit of detection
LR	Linear range
NAD ⁺	β - nicotinamide adenine dinucleotide
NIR	Near-infrared spectrophotometry
PMS-INT	Phenazine methosulphate-p-iodonitrotetrazolium violet
PTFE	Polytetrafluoroethylene

R.E.	Reference electrode
RSD	Relative standard deviation
SCE	Standard calomel electrode
W.E.	Working electrode

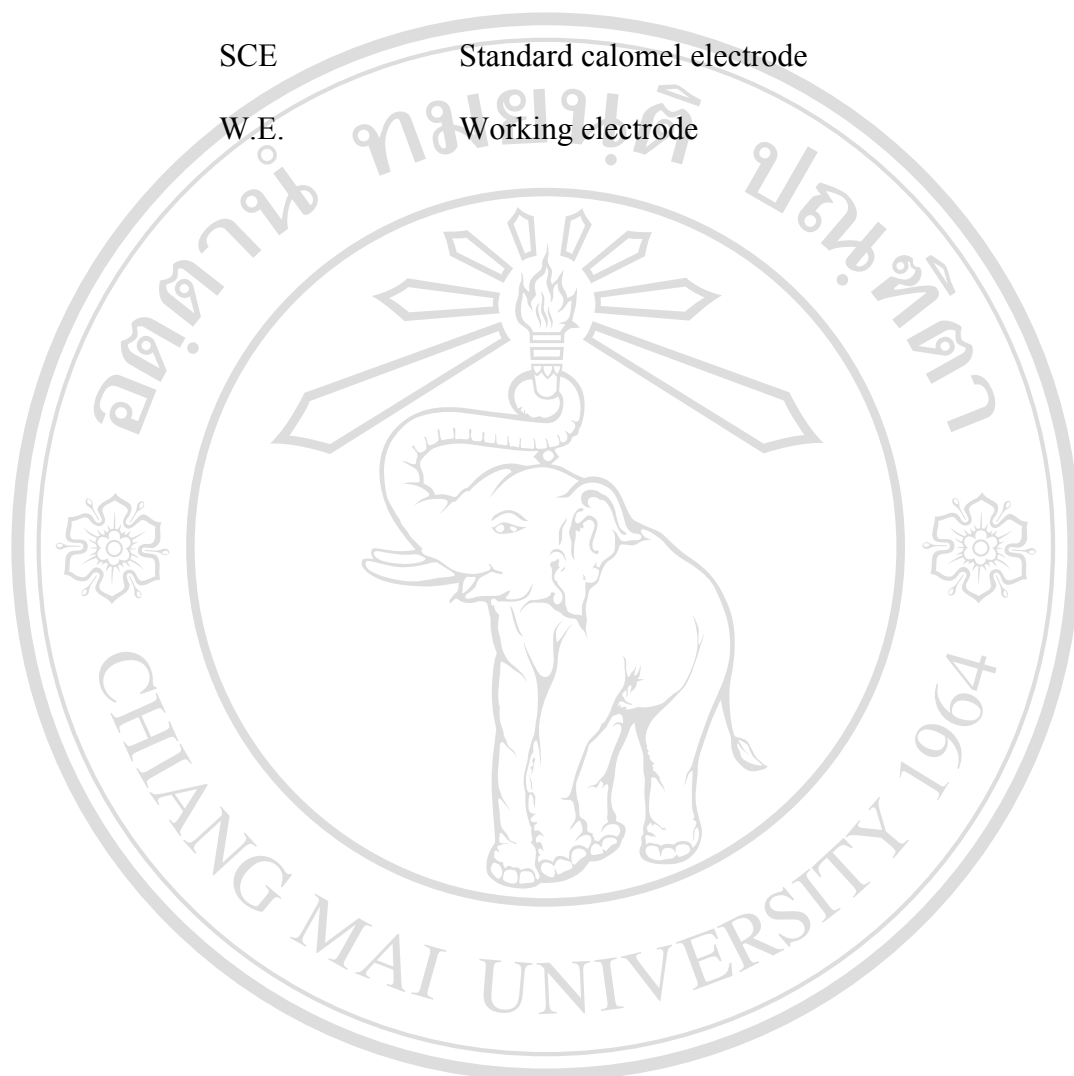

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่
Copyright © by Chiang Mai University
All rights reserved