

## TABLE OF CONTENTS

	Page
<b>ACKNOWLEDGEMENTS</b>	iii
<b>ABSTRACT (ENGLISH)</b>	iv
<b>ABSTRACT (THAI)</b>	vii
<b>TABLE OF CONTENTS</b>	x
<b>LIST OF TABLES</b>	xvii
<b>LIST OF FIGURES</b>	xxi
<b>ABBREVIATIONS AND SYMBOLS</b>	xxv
<b>CHAPTER I INTRODUCTION</b>	
1.1 Flow Injection Analysis (FIA)	1
1.1.1 Principle of FIA	2
1.1.2 Dispersion of sample zone	4
1.1.3 FIA Instrumentation	8
1.2 Sequential Injection Analysis (SIA)	10
1.2.1 Programmable Flow of SIA	12
1.2.2 Sequential Injection Analyzer	13
1.2.3 SIA Dispersion Zones	16

	<b>Page</b>
1.2.4 Mixing and Zone Overlap of SIA	18
1.3 Iron	20
1.3.1 Physical and Chemical Properties	20
1.3.2 Sources and Uses	21
1.3.3 Toxicity and Limiting Concentrations	21
1.3.4 Determination of Iron	22
1.4 Eriochrome cyanine R	25
1.5 Research Aims	29
 <b>CHAPTER II EXPERIMENTAL</b>	
2.1 Instruments and Apparatus	30
2.2 Chemicals	30
2.3 Preparation of Standard Solutions and Reagents	31
2.3.1 Preparation of Standard Solutions and Reagents of FIA system	32
2.3.1.1 Iron stock solution 1000 mg L <sup>-1</sup>	32
2.3.1.2 Eriochrome cyanine R solution 0.03 mol L <sup>-1</sup>	32
2.3.1.3 Cetyltrimethylammonium bromide stock solution 0.1 mol L <sup>-1</sup>	32
2.3.1.4 A 0.1 mol L <sup>-1</sup> of Acetate buffer pH 4.5	33

	<b>Page</b>
2.3.2 Preparation of standard solutions and reagents of SIA system	33
2.3.2.1 Iron stock solution 1000 mg L <sup>-1</sup>	33
2.3.2.2 Eriochrome cyanine R solution 0.03 mol L <sup>-1</sup>	33
2.3.2.3 Cetyltrimethylammonium bromide stock solution 0.1 mol L <sup>-1</sup>	33
2.3.2.4 A 0.1 mol L <sup>-1</sup> of Acetate buffer pH 4.5	34
2.4 Preliminary Studies of Spectrophotometric Determination of Iron (III) by Using Eriochrome cyanine R as Complexing Agent	34
2.4.1 Absorption spectra	34
2.4.2 Study of the composition of the Fe-ECR-CTMAB complex by Mole-ratio method	35
2.5 Procedure	35
2.5.1 Procedure for collection and treating drinking water samples for iron (III) determination	35
2.5.2 FIA spectrophotometric determination of iron (III) using ECR and CTMAB as complexing agent	36
2.5.2.1 Optimization of the flow system by univariate method	38
2.5.2.2 Linearity of calibration graph	39
2.5.2.3 Precision	40

	<b>Page</b>	
2.5.2.4	Detection limit	40
2.5.2.5	Accuracy of the proposed method	41
2.5.2.6	Interference studies	41
2.5.2.7	Validation method	42
2.5.3	SIA spectrophotometric determination of iron (III) using ECR and CTMAB as complexing agent	43
2.5.3.1	Sequential injection method	45
2.5.3.2	Optimization of the sequential injection system	47
2.5.3.3	Linearity of calibration graph	49
2.5.3.4	Precision	50
2.5.3.5	Detection limit	50
2.5.3.6	Accuracy of the proposed method	50
2.5.3.7	Interference studies	50
2.5.3.8	Validation method	51

### **CHAPTER III RESULTS AND DISCUSSION**

3.1	Preliminary Studies of Spectrophotometric Determination of Iron (III)	52
-----	---	----

by Using Eriochrome cyanine R as Complexing Agent

3.1.1	Absorption spectra	52
-------	--------------------	----

	<b>Page</b>
3.1.2 Mole-ratio method	53
3.2 FIA Spectrophotometric Determination of Iron (III) Using Eriochrome cyanine R and Cetyltrimethyl Ammonium Bromide as A Complexing Agent	58
3.2.1 Optimization of the Flow System by Univariate Method	58
3.2.1.1 Optimum wavelength	58
3.2.1.2 Effect of pH	60
3.2.1.3 Effect of ECR concentration	61
3.2.1.4 Effect of CTMAB concentration	63
3.2.1.5 Effect of flow rate	64
3.2.1.6 Effect of reaction coil length	66
3.2.1.7 Effect of sample volume	67
3.2.1.8 Summary of the studied range and optimum conditions	69
3.2.2 Analytical Characteristics of the method	69
3.2.2.1 Linear range	69
3.2.2.2 Calibration curve	72
3.2.2.3 Precision of the flow injection system	75
3.2.2.4 Detection limit	76
3.2.2.5 Interference Studies	77

	<b>Page</b>
3.2.2.6 Effect of masking agents and interference	83
3.2.2.7 Determination of iron (III) in drinking water samples	84
3.3 SIA Spectrophotometric Determination of Iron (III) Using Eriochrome cyanine R and Cetyltrimethyl Ammonium Bromide as A Complexing Agent	87
3.3.1 Study aspiration order	87
3.3.2 Optimization of the sequential injection system by univariate method	88
3.3.2.1 Effect of pH	89
3.3.2.2 Effect of pH concentration	90
3.3.2.3 Effect of ECR concentration	92
3.3.2.4 Effect of CTMAB concentration	93
3.3.2.5 Effect of aspiration volumes of acetate buffer	95
3.3.2.6 Effect of aspiration volumes of ECR	96
3.3.2.7 Effect of aspiration volumes of CTMAB	98
3.3.2.8 Effect of aspiration volumes of sample	99
3.3.2.9 Effect of flow rate	101
3.3.2.10 Effect of holding coil length	102
3.3.2.11 Effect of holding time	104

	<b>Page</b>
3.3.2.12 Effect of reaction coil length	105
3.3.2.13 Summary of the studied range and optimum conditions	107
3.3.3 Analytical Characteristics of the method	108
3.3.3.1 Linear range	108
3.3.3.2 Calibration curve	110
3.3.3.3 Precision of the sequential injection system	113
3.3.3.4 Detection limit	115
3.3.3.5 Interference Studies	116
3.3.3.6 Effect of masking agents and interference	121
3.3.3.7 Determination of iron (III) in drinking waters	122
<b>CHAPTER IV CONCLUSIONS AND SUGGESTION FOR FURTHER</b>	<b>124</b>
<b>WORK</b>	
<b>REFERENCES</b>	<b>128</b>
<b>APPENDIX A</b>	<b>133</b>
<b>APPENDIX B</b>	<b>135</b>
<b>CURRICULUM VITAE</b>	<b>141</b>
<b>THE RELEVANCY OF THE RESEARCH WORK IN THAILAND</b>	<b>142</b>



ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่

Copyright© by Chiang Mai University

All rights reserved



## LIST OF TABLES

<b>Table</b>	<b>Page</b>
1.1 A brief review of the methods for the determination of iron	22
1.2 A brief review of FIA and SIA for the determination of iron	25
1.3 A brief review of ECR reagent for the determination of some metals	27
2.1 Preliminary experimental conditions of FIA for studying optimum wavelength of Fe-ECR-CTMAB	38
2.2 The studied range for the optimization of all parameters of FIA	39
2.3 The device sequence for one full cycle of the SIA system	46
2.4 The studied range for the optimization of all parameters of SIA	48
2.5 Preliminary experimental conditions of SIA for studying optimum pH of Fe-ECR-CTMAB	49
3.1 Effect of ECR concentrations for mole-ratio of Fe-ECR-CTMAB complex	54
3.2 Effect of CTMAB concentrations for mole-ratio of Fe-ECR-CTMAB complex	55
3.3 Effect of wavelength on the sensitivity	59
3.4 Effect of pH on the sensitivity	60
3.5 Effect of concentration of ECR on the sensitivity	62
3.6 Effect of concentration of CTMAB on the sensitivity	63
3.7 Effect of flow rate on the sensitivity	65

<b>Table</b>	<b>Page</b>
3.8 Effect of reaction coil length on the sensitivity	66
3.9 Effect of sample volume on the sensitivity	68
3.10 Univariate optimization of chemical and FIA variables	69
3.11 Peak height at various iron concentrations for linearity check of the calibration graph	70
3.12 $\Delta$ Peak height for calibration curve	73
3.13 Precision verification using standard 0.1 mg L <sup>-1</sup> iron	76
3.14 The blank signal resulting from 12 injections	77
3.15 Effect of interference study for 0.1 mg L <sup>-1</sup> iron	78
3.16 Summary of the interference effects of some ions on the responses obtain from 0.1 mg L <sup>-1</sup> iron	82
3.17 Effect of masking agent for Al <sup>3+</sup> the response obtained from 0.1 mg L <sup>-1</sup> iron (III)	83
3.18 Determination of iron in drinking water sample by FIA method	85
3.19 Comparative determination of iron in drinking water sample by proposed FIA method and ICP-MS	86
3.20 Sensitivity at various aspiration orders	88
3.21 Effect of pH on the sensitivity	89
3.22 Effect of concentration of acetate buffer pH 5.5 on the sensitivity	91

<b>Table</b>	<b>Page</b>
3.23 Effect of various concentration of ECR on the sensitivity	92
3.24 Effect of various concentration of CTMAB on the sensitivity	94
3.25 Effect of various aspiration volume of 0.1 mol L <sup>-1</sup> of acetate buffer pH 5.5 on the sensitivity	95
3.26 Effect of various aspiration volume of 3.5×10 <sup>-4</sup> mol L <sup>-1</sup> of ECR on the sensitivity	97
3.27 Effect of various aspiration volume of 2.5×10 <sup>-3</sup> mol L <sup>-1</sup> of CTMAB on the sensitivity	98
3.28 Effect of various aspiration volume of sample on the sensitivity	100
3.29 Effect of various flow rate on the sensitivity	101
3.30 Effect of various holding coil length on the sensitivity	103
3.31 Effect of various holding time on the sensitivity	104
3.32 Effect of various reaction coil length on the sensitivity	106
3.33 Optimum conditions for ion determination	107
3.34 Linearity of iron determination	108
3.35 ΔPeak height for calibration curve	111
3.36 Precision verification using various concentrations of iron standard	114
3.37 The blank signal resulting from 12 injections	115
3.38 Interference studies for 0.2 mg L <sup>-1</sup> standard iron by SIA method	116

<b>Table</b>		<b>Page</b>
3.39	Summary of interference effects of some ions on the response obtained from 0.2 mg L <sup>-1</sup> by SIA method	120
3.40	Effect of masking agent for mask Al <sup>3+</sup> the response obtained from 0.2 mg L <sup>-1</sup> by SIA method	121
3.41	Determination of iron in drinking water sample by SIA method	122
3.42	Comparative determination of iron in drinking water sample by proposed SIA method and ICP-MS	123
4.1	Comparison of the analytical characteristics between FIA and SIA methods for iron determination	127

## LIST OF FIGURES

Figure		Page
1.1	The Schematic diagram of the basic FIA system	3
1.2	The analog output has the form of a FIA peak	3
1.3	General types of transport in closed tubes	4
1.4	Effects of convection and diffusion on concentration profiles of analyses at the detector	5
1.5	Dispersed sample zone in flow system	6
1.6	Relationship between the rollers of a peristaltic pump and the pump tubes	9
1.7	Sequence zone of SIA systems	11
1.8	Structure of injected zones and concentration profiles as seen by the detector	12
1.9	Structure flow diagram of a sequential injection analyzer	14
1.10	Dispersed sample zones of SIA system	16
1.11	Forward and reversal flow of SIA system	19
1.12	The structure of Eriochrome cyanine R	26
2.1	The experimental setup of the FIA system for the determination of iron (III)	37
2.2	The experimental setup of the SIA system for determination of iron (III)	44

<b>Figure</b>	<b>Page</b>
2.3 FIALab 5.0 for windows software	44
2.4 Schematic diagram of the device sequence for one cycle of the SIA system	45
3.1 The absorbance spectrum of ECR, ECR-CTMAB, Fe-ECR and Fe-ECR-CTMAB complexes	52
3.2 Mole-ratio study of Fe-ECR-CTMAB system; effect of ECR concentration.	54
3.3 Mole-ratio study of Fe-ECR-CTMAB system; effect of CTMAB concentration.	56
3.4 The reaction of Fe-ECR-CTMAB	57
3.5 Relationship between wavelength and sensitivity of the calibration curve	59
3.6 Relationship between pH and sensitivity of the calibration curve	61
3.7 Relationship between concentration of ECR and sensitivity of the calibration curve	62
3.8 Relationship between concentration of CTMAB and sensitivity of the calibration curve	64
3.9 Relationship between flow rate and sensitivity of the calibration curve	65
3.10 Relationship between reaction coil length and sensitivity of the calibration curve	67

<b>Figure</b>	<b>Page</b>
3.11 Relationship between sample volume and sensitivity of the calibration curve	68
3.12 Relationship between net peak height and concentration of iron	71
3.13 The calibration signal of FIA spectrophotometric determination of iron 0.01-0.35 mg L <sup>-1</sup> and 0.50–0.80 mg L <sup>-1</sup>	74
3.14 The calibration curve of FIA spectrophotometric determination of iron: (a) iron 0.01-0.35 mg L <sup>-1</sup> ; (b) iron 0.50–0.80 mg L <sup>-1</sup>	75
3.15 Relationship between various pH and sensitivity of the calibration curve	90
3.16 Relationship between various concentration of acetate buffer pH 5.5 and sensitivity of the calibration curve	91
3.17 Relationship between various concentration of ECR solution and sensitivity of the calibration curve	93
3.18 Relationship between concentration of CTMAB on the sensitivity of the calibration curve	94
3.19 Relationship between various aspiration volume of 0.1 mol L <sup>-1</sup> of acetate buffer pH 5.5 on the sensitivity of the calibration curve	96
3.20 Relationship between various aspiration volumes of 3.5×10 <sup>-4</sup> mol L <sup>-1</sup> of ECR on the sensitivity of the calibration curve	97

<b>Figure</b>	<b>Page</b>
3.21 Relationship between various aspiration volumes of $2.5 \times 10^{-3} \text{ mol L}^{-1}$ of CTMAB on the sensitivity of the calibration curve	99
3.22 Relationship between various aspiration volumes of sample on the sensitivity of the calibration curve	100
3.23 Relationship between various flow rate on the sensitivity of the calibration curve	102
3.24 Relationship between various holding coil length on the sensitivity of the calibration curve	103
3.25 Relationship between various holding time on the sensitivity of the calibration curve	105
3.26 Relationship between various reaction coil length on the sensitivity of the calibration curve	106
3.27 Relationship between net peak height and concentration of iron	110
3.28 Calibration signal of SIA spectrophotometric determination of iron 0.02-0.45 $\text{mg L}^{-1}$ and 0.45-1.0 $\text{mg L}^{-1}$	112
3.29 The Calibration curve of SIA spectrophotometric determination of iron: (a) iron 0.02-0.45 $\text{mg L}^{-1}$ ; (b) iron 0.45-1.0 $\text{mg L}^{-1}$	113




## ABBREVIATIONS AND SYMBOLS

AU	absorbance unit
FIA	flow injection analysis
h	hour
i.d.	inner diameter
in.	inch
L	liter
LOD	limit of detection
LOQ	limit of quantitation
mg	milligram
min	minute
mL	milliliter
mm	millimeter
PC	personal computer
PTFE	polytetrafluoroethylene
$\bar{x}$	mean
P.H.	peak height
RSD	relative standard deviation

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่

Copyright © by Chiang Mai University

All rights reserved

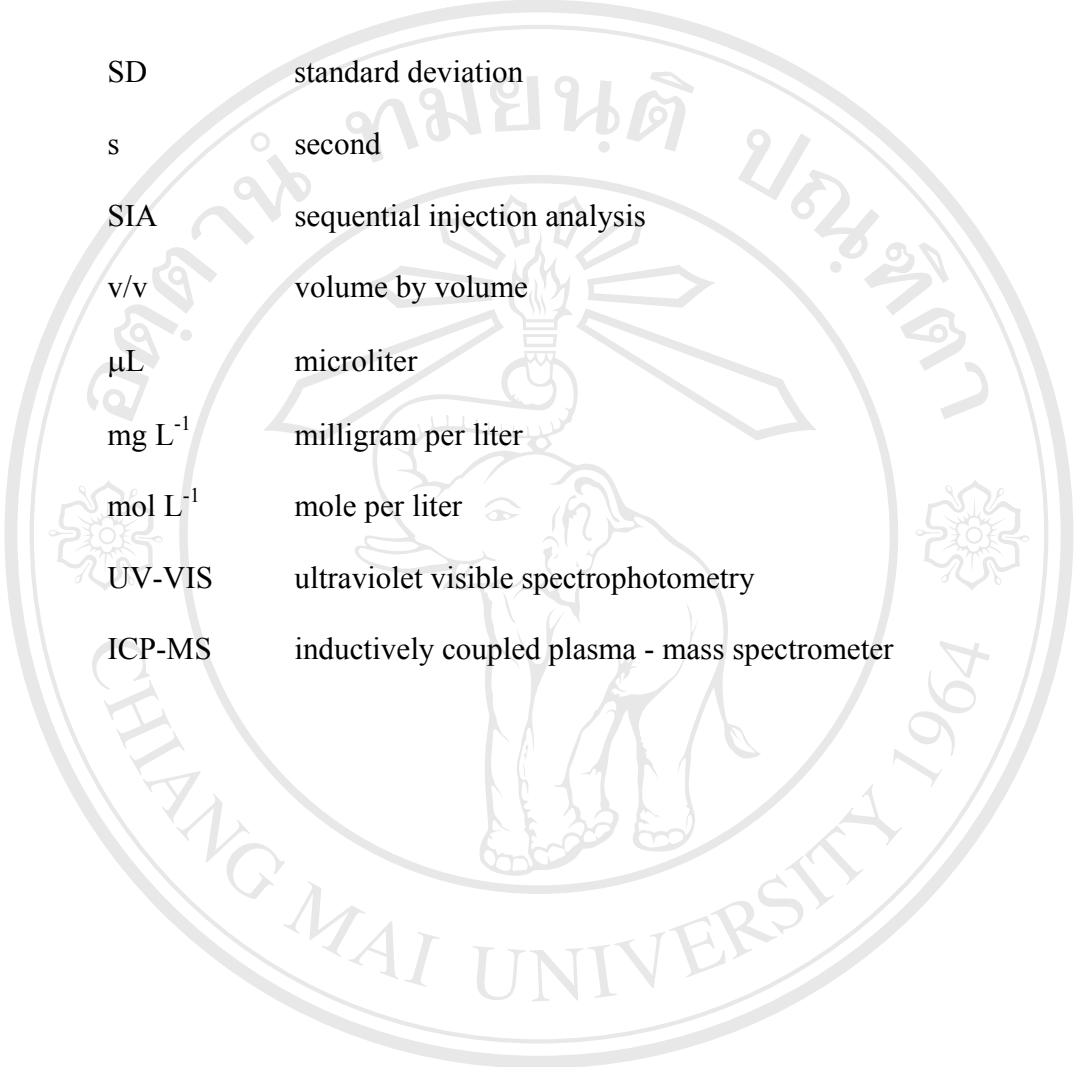

SD	standard deviation
s	second
SIA	sequential injection analysis
v/v	volume by volume
$\mu\text{L}$	microliter
$\text{mg L}^{-1}$	milligram per liter
$\text{mol L}^{-1}$	mole per liter
UV-VIS	ultraviolet visible spectrophotometry
ICP-MS	inductively coupled plasma - mass spectrometer

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่

Copyright© by Chiang Mai University

All rights reserved