

TABLE OF CONTENTS

	Page
ACKNOWLEDGEMENTS	iii
ABSTRACT (ENGLISH)	iv
ABSTRACT (THAI)	v
TABLE OF CONTENTS	vi
LIST OF TABLES	x
LIST OF FIGURES	xii
ABBREVIATIONS AND SYMBOLS	xiii
CHAPTER 1 INTRODUCTION	
1.1 Overview	1
1.2 Antioxidant and its important	2
1.3 Method for estimation of antioxidant	
1.3.1 Chromatographic methods	4
1.3.2 Methods based on the neutralization of free radical	8
1.3.3 Spectrophotometric methods	11
1.3.4 Electroanalytical methods	15
1.3.5 Flow analysis methods	18
1.4 Research objectives	23

CHAPTER 2 EXPERIMENTAL

2.1 Chemicals	24
2.2 Materials and instruments	25
2.3 Software	25
2.4 Preparation of standard solution and reagents	
2.4.1 Working standard solution of ascorbic acid	25
2.4.2 Reagents solution	
2.4.2.1 Potassium iodate solution in hydrochloric acid solution	26
2.4.2.2 Potassium iodide solution	26
2.5 Preparation of electrode	26
2.6 Manifold of flow injection amperometric method	26
using triiodide as a reagent for estimation of antioxidant activity	
2.7 Optimization of flow injection amperometric method	
using triiodide as a reagent	
2.7.1 Concentration of iodate	28
2.7.2 Concentration of potassium iodide	28
2.7.3 Concentration of hydrochloric acid	29
2.7.4 Total flow rate	30
2.8 Analytical characteristics of the procedure	
2.8.1 Calibration curves and limit of quantitative	30
2.8.2 Precision study	31
2.8.3 Recovery study	31
2.8.4 Interferences study	32

2.9 Sample analysis	
2.9.1 Preparation of sample	32
2.9.2 Precision study of sample extraction method	32
2.9.3 Comparison with FI – ferrous tartrate method	32
2.9.4 Comparison with FI – colorimetric method based on FRAP reaction method	33
2.9.5 Application of the method to real samples	33

CHAPTER 3 RESULTS AND DISSCUSSION

3.1 Optimization of flow injection amperometric method using triiodide as a reagent	
3.1.1 Concentration of iodate	36
3.1.2 Concentration of potassium iodide	37
3.1.3 Concentration of hydrochloric acid	37
3.1.4 Total flow rate	38
3.1.5 Summary of the selected conditions	39
3.2 Analytical characteristics of the procedure	
3.2.1 Calibration curves and limit of quantitative	40
3.2.2 Precision study	41
3.2.3 Recovery study	43
3.2.4 Interferences study	45
3.3 Sample analysis and comparison to other methods	48
CHAPTER 4 CONCLUSION	55

REFERENCES	57
APPENDICES	62
Appendix A Flow injection analysis	63
Appendix B Amperometric method	65
Appendix C FI-ferrous tartrate method	68
Appendix D FI – colorimetric method based on FRAP reaction	70
Appendix E Structure of some antioxidant compounds	71
THE RELEVANCY OF THE RESEARCH WORK TO THAILAND	75
CURRICULUM VITAE	76

LIST OF TABLES

Table		Page
1.1	Summary of some chromatographic methods for the determination of antioxidant	5
1.2	Summary of some methods based on the neutralization of free radical	10
1.3	The summary of some spectrophotometric methods for the estimation of antioxidant activity	13
1.4	The summary of some electrochemical methods for the estimation of antioxidant activity	16
1.5	Some analytical methods based on with the flow injection system for estimation of antioxidant	19
2.1	The conditions for the study of effect of potassium iodate concentration	28
2.2	The conditions for the study of effect of potassium iodide concentration	29
2.3	The conditions for the study of effect of hydrochloric concentration	29
2.4	The conditions for the study of effect of total flow rate	30
3.1	The optimum condition of FI-amperometric method for estimation of antioxidant activity	39
3.2	The precision of the system at two concentration of ascorbic acid	42
3.3	The precision study of the sample preparation method	43

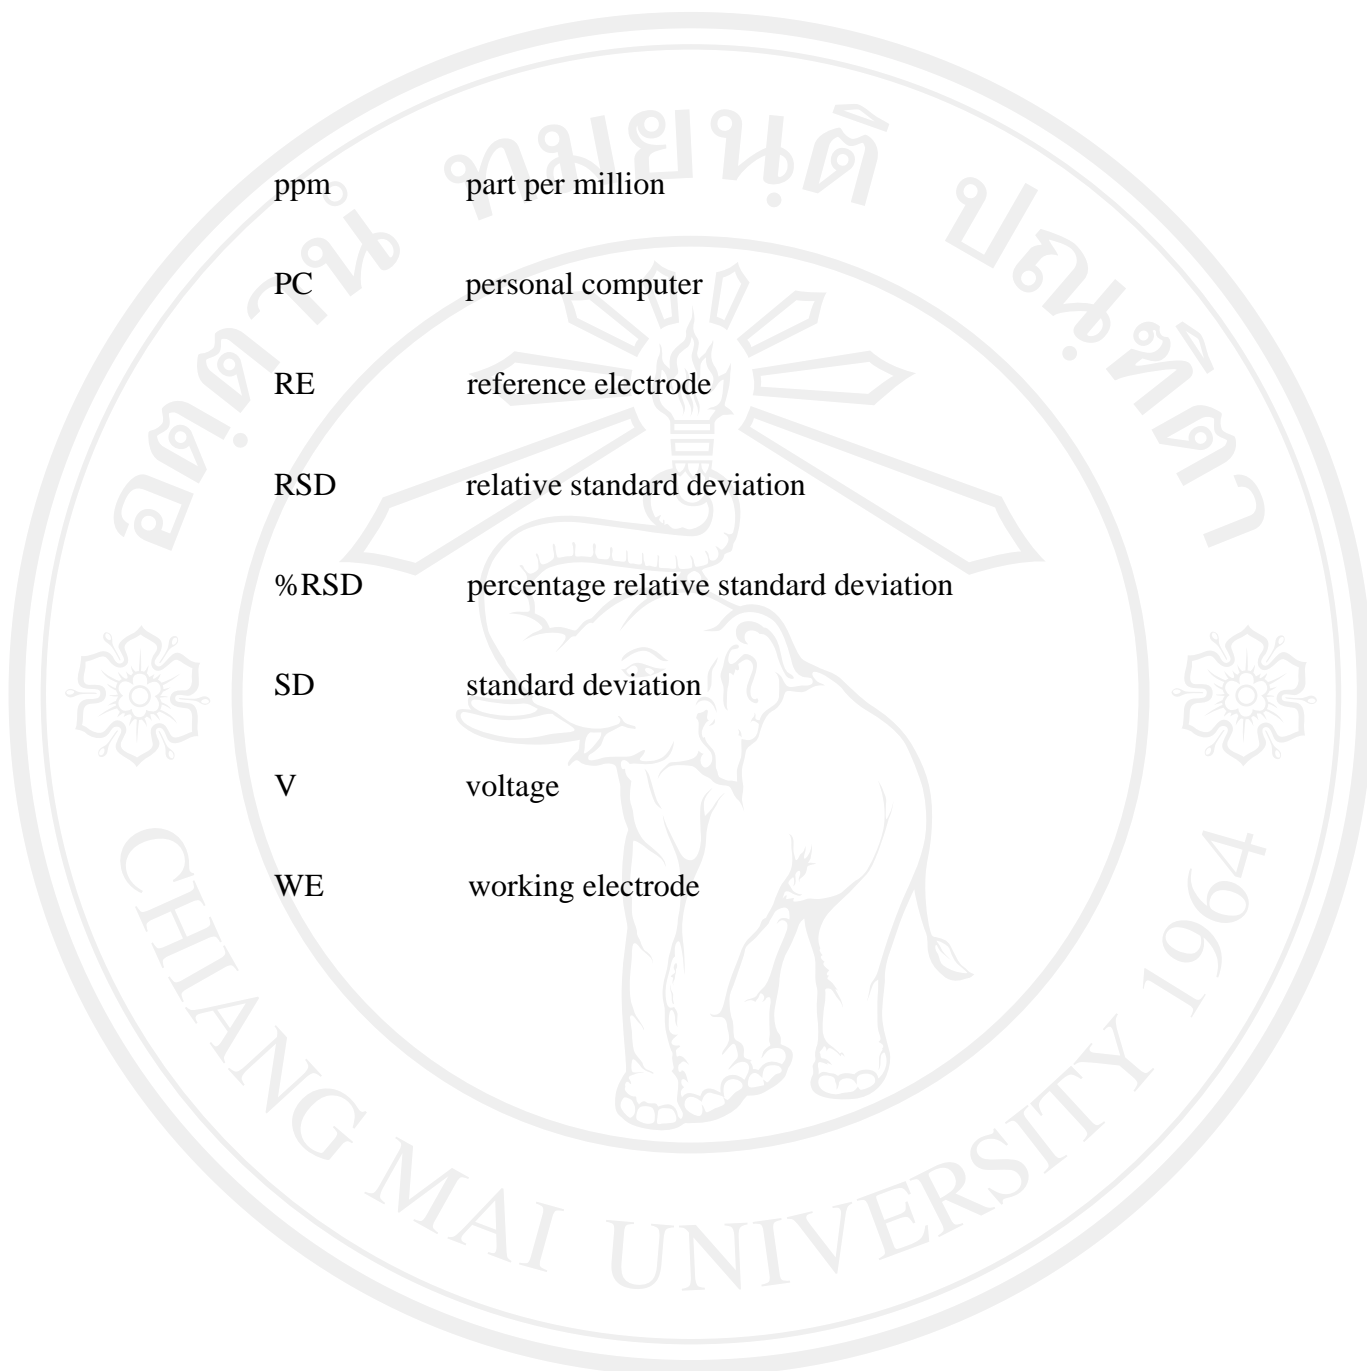
3.4	The recovery percentages obtained by spiking ascorbic acid at 10-40 ppm into sample	44
3.5	Comparisons content of antioxidant between calculated from standard addition graph and calibration graph	45
3.6	Summary of the percentage of recovery at various ratio of interference to ascorbic acid	46
3.7	Antioxidant content in some tea infusion samples	49
3.8	Antioxidant content in some tea infusion samples	52

LIST OF FIGURES

Figure		Page
1.1	DPPH and ABTS structure	9
2.1	Manifold for the Estimation of Antioxidant Activity	27
3.1	Effect of potassium iodate concentration on sensitivity of the method	36
3.2	Effect of potassium iodide concentration on sensitivity of the method	37
3.3	Effect of hydrochloric acid concentration on sensitivity of the method	38
3.4	Effect of total flow rate on sensitivity of the method	39
3.5	FI-Agram for the estimation of antioxidant activity by FI-amperometric method.	40
3.6	Calibration graph for the estimation of antioxidant activity by FI-amperometric method	41
3.7	Correlation graph of antioxidant contents obtained by the proposed method and FI-ferrous tartrate method	51
3.8	Correlation graph of antioxidant contents by the proposed method and FI – colorimetric method based on FRAP reaction	54

ABBREVIATIONS AND SYMBOLS

AA	ascorbic acid
cm	centimeter
FC	electrochemical flow cell
FIA, FI	flow injection analysis
g	gram
GC	gas chromatography
GCE	glassy carbon working electrode
h ⁻¹	per hour
HPLC	high performance liquid chromatography
L	liter
LC	liquid chromatography
μM	micro molarity
mL	milliliter
mL.min ⁻¹	milliliter per minute
M	Molarity
MS	mass spectrometry

The background of the page features a large, light gray watermark of the Chiang Mai University logo. The logo is circular and contains the Thai text 'มหาวิทยาลัยเชียงใหม่' at the top and 'CHIANG MAI UNIVERSITY 1964' at the bottom. In the center of the logo is an elephant standing under a sunburst. The table of abbreviations is overlaid on this watermark.

ppm	part per million
PC	personal computer
RE	reference electrode
RSD	relative standard deviation
%RSD	percentage relative standard deviation
SD	standard deviation
V	voltage
WE	working electrode