

## TABLE OF CONTENTS

	<b>Page</b>
<b>ACKNOWLEDGEMENTS</b>	iii
<b>ABSTRACT (ENGLISH)</b>	iv
<b>ABSTRACT (THAI)</b>	vi
<b>TABLE OF CONTENTS</b>	viii
<b>LIST OF TABLES</b>	xii
<b>LIST OF FIGURES</b>	xv
<b>ABBREVIATIONS AND SYMBOLS</b>	xviii
<b>CHAPTER 1 INTRODUCTION</b>	<b>1</b>
1.1 Overview of human hair sample	1
1.1.1 The structure of hair	2
1.1.2 Hair growth	3
1.1.3 Mechanisms of metal incorporation into hair	4
1.1.4 The advantages of human hair samples	5
1.2 Ultrasonic acid digestion	6
1.2.1 History of ultrasonic energy	6
1.2.2 Ultrasonic bath	8
1.2.3 Parameters affecting ultrasonic cavitation	9
1.2.4 Applications of ultrasonic	12

	<b>Page</b>
1.3 Cloud point extraction	14
1.3.1 History of cloud point extraction	14
1.3.2 Theory of cloud point extraction	15
1.3.3 The advantages of cloud point extraction	16
1.3.4 Influential parameters	17
1.3.5 Implementation of CPE in metal analysis	20
1.4 Atomic absorption spectrometry (AAS)	22
1.4.1 Theory of atomic absorption spectrometry	22
1.4.2 Flame atomic absorption spectrometry	24
1.5 Literature review	26
1.6 Research objectives	28
<b>CHAPTER 2: EXPERIMENTAL</b>	<b>29</b>
2.1 Chemicals and apparatus	29
2.1.1 Chemicals	29
2.1.2 Apparatus	29
2.2 Preparation standard solutions and reagents	30
2.3 Analytical characteristics of the method	32
2.4 Preparation of human hair samples	34
2.5 Ultrasonic acid digestion (UAD) method	35
2.6 Cloud point extraction (CPE) procedure	37
2.7 Determination of chromium,nickel and lead in human hair samples	41

	<b>Page</b>
<b>CHAPTER 3 RESULTS AND DISCUSSION</b>	<b>45</b>
3.1 Analytical characteristics of the method	46
3.1.1 Precision	46
3.1.2 Limit of Detection (LOD) and Limit of quantitation (LOQ)	47
3.1.3 Accuracy	48
3.2 Optimization of ultrasonic acid digestion (UAD)	50
3.2.1 Effect of solvent systems	51
3.2.2 Effect of presonication time	54
3.2.3 Effect of sonication time	56
3.2.4 Effect of temperature of the ultrasonic bath	60
3.2.5 Optimum conditions of ultrasonic acid digestion	62
3.3 Optimization of cloud point extraction (CPE)	63
3.3.1 Effect of pH	65
3.3.2 Effect of APDC concentration	66
3.3.3 Effect of Triton X-114 concentration	70
3.3.4 Effects of equilibration time	73
3.3.5 Effects of equilibration temperature	75
3.3.6 Optimum conditions of cloud point extraction	77
3.4 Determination of cadmium and lead in human hair samples	79
<b>CHAPTER 4 CONCLUSION</b>	<b>83</b>
<b>REFERENCES</b>	<b>86</b>

	<b>Page</b>
<b>APPENDICES</b>	<b>91</b>
APPENDIX A Calibration curve by FAAS detection	92
APPENDIX B Precision and detection limit of chromium, nickel and lead by FAAS detection	95
<b>CURRICURUM VITAE</b>	<b>100</b>

## LIST OF TABLES

<b>Table</b>	<b>Page</b>
2.1 The concentrations of lead, chromium and nickel standard solutions for FAAS determination	32
2.2 The conditions for optimization of ultrasonic acid digestion	38
2.3 The conditions for optimization of cloud point extraction	41
2.4 Operating conditions for ultrasonic acid digestion of Cr, Ni and Pb from human hair samples	42
2.5 The conditions for preconcentration of Cr, Ni and Pb in human hair samples	43
2.6 Instrument settings and analytical conditions of Cr, Ni and Pb in FAAS	43
2.7 Human hair samples from various cases	44
3.1 Operating parameters and analytical conditions of Cr, Ni and Pb in FAAS	45
3.2 The precision of the FAAS instrument for Cr, Ni and Pb analysis	46
3.3 Absorbance obtained from blank solution	47
3.4 The recoveries of Cr analysis	48
3.5 The recoveries of Ni analysis	49
3.6 The recoveries of Pb analysis	50
3.7 The effect of solvent system on the analytical signal of $3 \mu\text{g ml}^{-1}$ Ni, $2 \mu\text{g ml}^{-1}$ Cr and $10 \mu\text{g ml}^{-1}$ Pb	53
3.8 The effect of presonication time on the analytical signal of $3 \mu\text{g ml}^{-1}$ Ni, $2 \mu\text{g ml}^{-1}$ Cr and $10 \mu\text{g ml}^{-1}$ Pb	55

3.9	The effect of sonication time on the analytical signal of $3 \mu\text{g ml}^{-1}$ Ni, $2 \mu\text{g ml}^{-1}$ Cr and $10 \mu\text{g ml}^{-1}$ Pb	58
3.10	The effect of temperature of the ultrasonic bath on the analytical signal of $3 \mu\text{g ml}^{-1}$ Ni, $2 \mu\text{g ml}^{-1}$ Cr and $10 \mu\text{g ml}^{-1}$ Pb	60
3.11	Operating conditions for ultrasonic acid digestion of Cr, Ni and Pb from human hair samples	62
3.12	The effect of pH on the analytical signal for Cr, Ni and Pb	65
3.13	The effect of APDC concentration on the analytical signal for Cr, Ni and Pb	68
3.14	The effect of Triton X-114 concentration on the analytical signal for Cr, Ni and Pb	71
3.15	The effect of complexing time on the analytical signal for Cr, Ni and Pb	73
3.16	The effect of equilibration temperature on the analytical signal for Cr, Ni and Pb	75
3.17	Optimum conditions of cloud point extraction	77
3.18	The amount of Cr, Ni and Pb in human hair samples	80
A-1	Calibration equation and $R^2$ used for study on ultrasonic acid digestion of Cr from FAAS	93
A-2	Calibration equation and $R^2$ used for study on cloud point extraction of Cr from FAAS	93
A-3	Calibration equation and $R^2$ used for study on ultrasonic acid digestion of Ni from FAAS	94

A-4	Calibration equation and $R^2$ used for study on cloud point extraction of Ni from FAAS	94
A-5	Calibration equation and $R^2$ used for study on ultrasonic acid digestion of Pb from FAAS	95
A-6	Calibration equation and $R^2$ used for study on cloud point extraction of Pb from FAAS	95
B-1	The concentration of Cr in human hair samples	97
B-2	The concentration of Ni in human hair samples	98
B-3	The concentration of Pb in human hair samples	99
B-4	The amount of Cr, Ni and Pb in human hair samples	100

## LIST OF FIGURES

<b>Figure</b>	<b>Page</b>
1.1 (a) cross-section and (b) structure of a hair shaft in a hair follicle in the skin	2
1.2 Diagram illustrating hair growth sequences	4
1.3 Possible model for metal incorporation into hair	5
1.4 Ultrasonic bath for operation at frequencies of 20 – 80 kHz	8
1.5 The cavitation bubble at frequencies of 20 – 80 kHz	10
1.6 Cavitation collapse at a solid-liquid interface. The sequence (1), (2) and (3) shows a scheme of fragmentation or disruption due to gas trapped on the defects on the solid surface giving rise to particle-size reduction	13
1.7 Micelle formation with increasing surfactant concentration	16
1.8 The experimental procedure for CPE in metal analysis	21
1.9 Schematic of FAAS	25
2.1 The human hair samples	34

2.2	The flow chart of hair washing	35
2.3	The flow chart of ultrasonic acid digestion	36
2.4	The flow chart of cloud point extraction procedure	39
3.1	Operating parameters and analytical conditions of Cr, Ni and Pb in FAAS	45
3.2	The sample solution with various volume of H <sub>2</sub> O <sub>2</sub>	52
3.3	Effect of volume of H <sub>2</sub> O <sub>2</sub> on the analytical signal of 3 µg ml <sup>-1</sup> Ni, 2 µg ml <sup>-1</sup> Cr and 10 µg ml <sup>-1</sup> Pb	53
3.4	The human hair sample was added with acid mixtures and kept at room temperature	54
3.5	Effect of presonication time on the analytical signal of 3 µg ml <sup>-1</sup> Ni, 2 µg ml <sup>-1</sup> Cr and 10 µg ml <sup>-1</sup> Pb	56
3.6	Presonication of digested hair sample for 10 minute (left) and sonication sample for 30 minute (right)	57
3.7	Effect of sonication time on the analytical signal of 3 µg ml <sup>-1</sup> Ni, 2 µg ml <sup>-1</sup> Cr and 10 µg ml <sup>-1</sup> Pb	61
3.8	Effect of ultrasonic bath temperature on the analytical signal of 3 µg ml <sup>-1</sup> Ni, 2 µg ml <sup>-1</sup> Cr and 10 µg ml <sup>-1</sup> Pb	63
3.9	The prior formation of metal ions and chelating agent in CPE	64
3.10	Effect of pH on the cloud point extraction of 3 µg ml <sup>-1</sup> Ni, 2 µg ml <sup>-1</sup> Cr and 10 µg ml <sup>-1</sup> Pb	66
3.11	Structure of metal-APDC complex	67

3.12 Effect of APDC concentration on the cloud point extraction of 3 $\mu\text{g ml}^{-1}$ Ni, 2 $\mu\text{g ml}^{-1}$ Cr and 10 $\mu\text{g ml}^{-1}$ Pb	69
3.13 Structure of Triton X-114 surfactant	70
3.14 The micelle formation of surfactant	70
3.15 Effect of Triton X-114 concentration on the cloud point extraction of 3 $\mu\text{g ml}^{-1}$ Ni, 2 $\mu\text{g ml}^{-1}$ Cr and 10 $\mu\text{g ml}^{-1}$ Pb	72
3.16 The effect of complexing time on the cloud point extraction of 3 $\mu\text{g ml}^{-1}$ Ni, 2 $\mu\text{g ml}^{-1}$ Cr and 10 $\mu\text{g ml}^{-1}$ Pb	74
3.17 The effect of equilibration temperature on the cloud point extraction of 3 $\mu\text{g ml}^{-1}$ Ni, 2 $\mu\text{g ml}^{-1}$ Cr and 10 $\mu\text{g ml}^{-1}$ Pb	76

## ABBREVIATIONS AND SYMBOLS

AAS	atomic absorption spectrophotometry
FAAS	flame atomic absorption spectrophotometry
Abs.	absorbance
Conc.	concentration
°C	degree Celsius
Vol.	volume
Cal	calculation
g	gram
ppm	parts per million
hr	hour
mol l <sup>-1</sup>	mol per liter
µg ml <sup>-1</sup>	microgram per milliliter
µl	microliter
mg	milligram
ml	milliliter
min	minute
%	percentage
RSD	relative standard deviation
SD	standard deviation
% v/v	percentage of volume by volume


$R^2$  correlation coefficient

cm centimeter

rpm round per minute

$\text{g mol}^{-1}$  gram per mol

l/min liter per minute

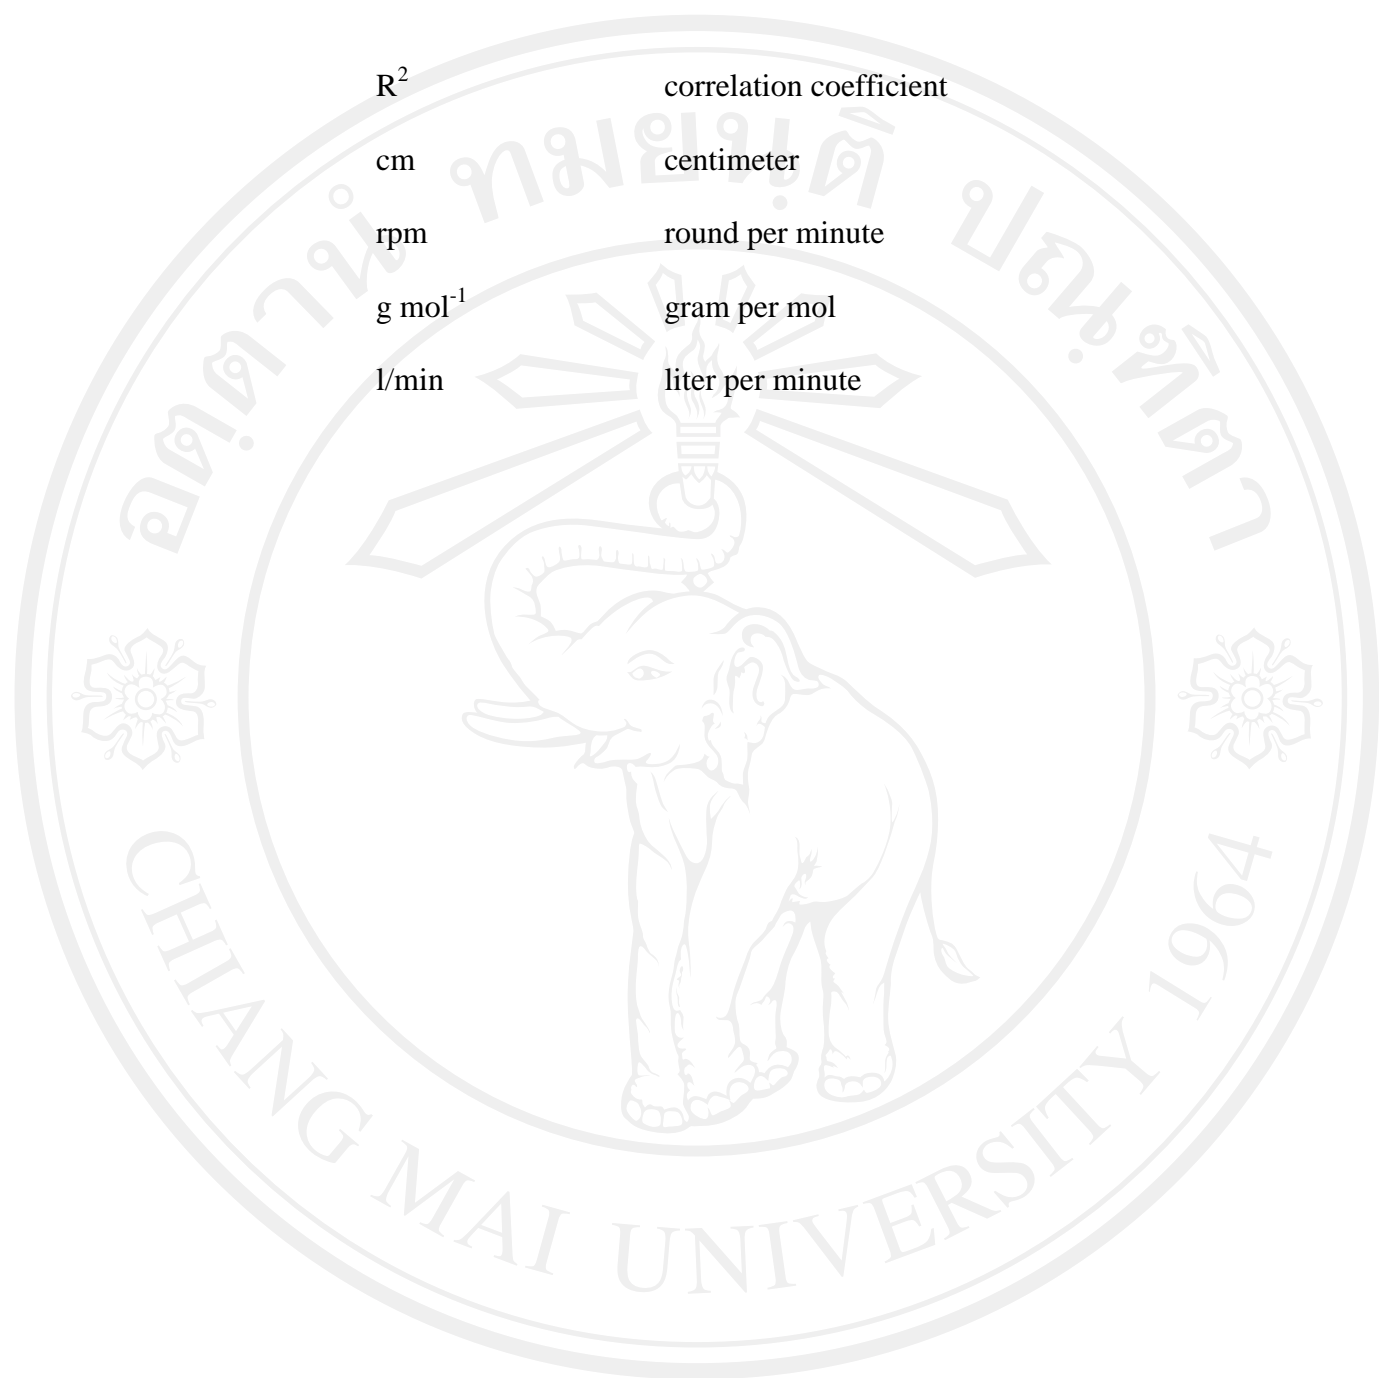

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่

Copyright© by Chiang Mai University  
All rights reserved