

CONTENTS

	Page
Acknowledgments	c
Abstract in Thai	e
Abstract in English	g
List of Tables	m
List of Figures	n
List of Abbreviations	p
List of Symbols	r
Chapter 1 Introduction	
1.1 Overview	1
1.2 Hydroquinone	2
1.3 Flow injection analysis	4
1.4 Amperometric method	6
1.5 Screen-printed electrode	7
1.6 Hydroquinone biosensor	11
1.7 Enzyme immobilization method	13
1.8 Research objectives	17

Chapter 2 Experimental

2.1 Chemicals	18
2.2 Materials and instruments	19
2.3 Software	20
2.4 Preparation of reagents	20
2.5 Preparation of electrode	21
2.6 Working electrode investigation	21
2.7 Study on effect of CNTs amount	22
2.8 Characterization of the electrode surface	22
2.9 Manifold of flow injection amperometric system	22
2.10 Optimization of flow injection amperometric system	23
2.11 Procedure for laccase column preparation	24
2.12 Testing efficiency of the laccase column	25
2.13 Optimization of the parameters of the biosensor	
2.13.1 Effect of flow rate	26
2.13.2 Effect of pH	26
2.13.3 Effect of buffer concentration	27
2.13.4 Effect of temperature	27
2.14 Analytical characteristics of the procedure	
2.14.1 Calibration graph and detection limit	28
2.14.2 Precision study	28
2.14.3 Stability of biosensor	29

2.14.4 Interference study	29
2.14.5 Real samples analysis	30

Chapter 3 Results and Discussion

3.1 Working electrode investigation	31
3.2 Effect of CNTs amount	33
3.3 Characterization of the electrode surface	34
3.4 Optimization of flow injection amperometric system	
3.4.1 Effect of applied potential	35
3.4.2 Effect of sample volume	36
3.4.3 Effect of mixing coil length	37
3.5 Testing efficiency of the laccase column	38
3.6 Optimization of the parameters of the biosensor	
3.6.1 Effect of flow rate	41
3.6.2 Effect of pH	42
3.6.3 Effect of buffer concentration	43
3.6.4 Effect of temperature	44
3.7 Analytical characteristics of the procedure	
3.7.1 Calibration graph and detection limit	44
3.7.2 Precision study	46
3.7.3 Stability of biosensor	48
3.7.4 Interference study	49

3.7.5 Real samples analysis	50
Chapter 4 Conclusion	54
References	56
List of publication	66
Appendix A	67
Appendix B	71
Curriculum Vitae	74



ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่
Copyright© by Chiang Mai University
All rights reserved

LIST OF TABLES

	Page
Table 1.1 Some analytical methods for determination of hydroquinone	3
Table 1.2 Some reports of application of carbon electrode modified with different materials	9
Table 1.3 Some reports of the methods for enzyme immobilization	15
Table 2.1 The conditions for the study of each parameter	24
Table 2.2 The conditions for the study of effect of flow rate	26
Table 2.3 The conditions for the study of effect of pH	26
Table 2.4 The conditions for the study of effect of buffer concentration	27
Table 2.5 The conditions for the study of effect of temperature	27
Table 3.1 The peak height signal obtained of 10 μ M quinone from 9 modified electrodes	47
Table 3.2 Interfering effect of the studied substances on the FI-Amp sensor	49
Table 3.3 The percentage of recovery at various spiked hydroquinone concentration into water samples	51

LIST OF FIGURES


	Page
Figure 1.1 The simplest flow injection system	5
Figure 1.2 The mechanism of hydroquinone biosensor	12
Figure 2.1 FI manifold of flow injection amperometric system for determination of hydroquinone; carrier = 0.1 M citrate buffer, I = injection valves, S = standard/ sample, C = laccase column, M = mixing coil, EC = electrochemical cell (WE, RE and AE), W = waste, D = amperometer and PC = personal computer	23
Figure 2.2 The laccase column	25
Figure 3.1 Cyclic voltammograms on CNTs modified SPCE of 0.1 to 2 mM quinone in 0.1 M citrate buffer pH 5	32
Figure 3.2 The sensitivity of the various electrodes with 0.1 to 2 mM quinone in 0.1 M citrate buffer pH 5	33
Figure 3.3 The effect of volume of CNTs with 0.1 to 2 mM quinone	34
Figure 3.4 SEM images of (A) bare SPCE and (B) SPCE modified with CNTs	34
Figure 3.5 Effect of the applied working potential for reduction of quinone on sensitivity of 5 to 20 μ M hydroquinone	36

Figure 3.6	Effect of sample volume on sensitivity of 5 to 20 μM hydroquinone	37
Figure 3.7	Effect of mixing coil length on sensitivity of 5 to 20 μM hydroquinone	38
Figure 3.8	FIAGram of the signal of 10 μM hydroquinone obtained from the FI-Amp system with and without the laccase column	39
Figure 3.9	The signal of hydroquinone in the range of 1–100 μM obtained from the system without the laccase column	39
Figure 3.10	The signal of hydroquinone in the range of 1–100 μM obtained from the system with the laccase column	40
Figure 3.11	Calibration graph of hydroquinone in the range of 1–50 μM	40
Figure 3.12	Effect of flow rate on sensitivity of 5 to 20 μM hydroquinone	42
Figure 3.13	Effect of pH on sensitivity of 5 to 20 μM hydroquinone	43
Figure 3.14	Effect of citrate buffer concentration on sensitivity of 5 to 20 μM hydroquinone	43
Figure 3.15	Effect of temperature on sensitivity of 5 to 20 μM hydroquinone	44
Figure 3.16	FIAGram of signal response to hydroquinone concentration from 1 to 50 μM using the FI-Amp sensor	45
Figure 3.17	Calibration graph obtained in the range of 1–50 μM hydroquinone	46
Figure 3.18	The stability of the biosensor for hydroquinone measurement in a period of 30 days	48
Figure 5.1	<i>Trametes versicolor</i>	71
Figure 5.2	Copper binding residues of laccase enzyme	73

LIST OF ABBREVIATIONS

AE	Auxiliary electrode
AuNPs	Gold nanoparticles
CNTs	Carbon nanotubes
CPE	Carbon paste electrode
DI	Deionized
EC	Electrochemical cell
FI	Flow injection
FIA	Flow injection analysis
FI-Amp	Flow injection amperometric
GCE	Glassy carbon electrode
GE	Graphite electrode
HPLC	High performance liquid chromatography
HQ	Hydroquinone
I.D.	Inner diameter
LOD	Limit of detection
MWCNTs	Multi-wall carbon nanotubes
O.D.	Outer diameter
PC	Personal computer
PMMA	Poly(methyl methacrylate)

RE	Reference electrode
RSD	Relative standard deviation
SEM	Scanning electron microscope
SD	Standard deviation
SPCE	Screen-printed carbon electrode
SPE	Screen-printed electrode
SWCNTs	Single-wall carbon nanotubes
WE	Working electrode

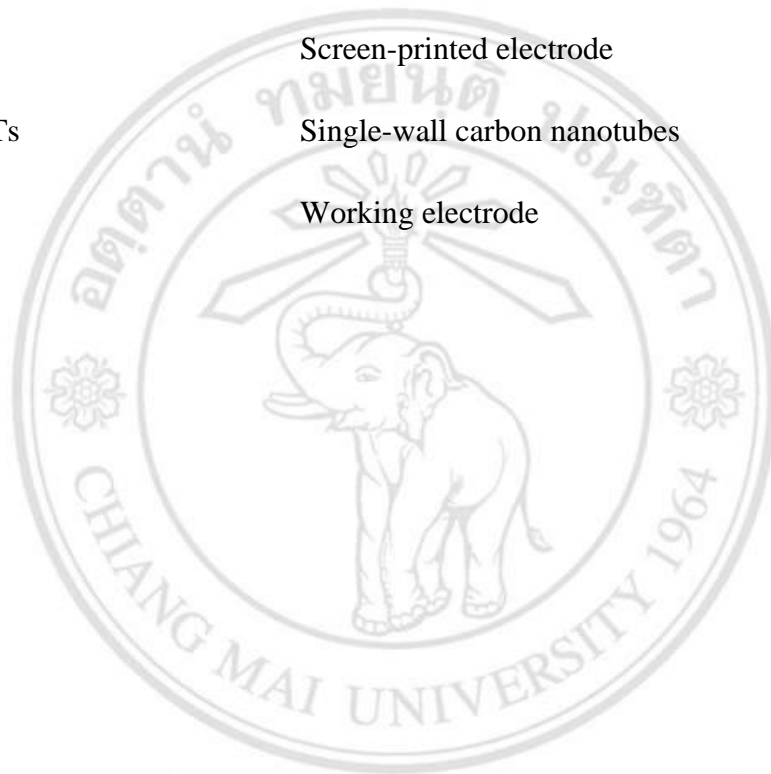

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่
 Copyright© by Chiang Mai University
 All rights reserved

LIST OF SYMBOLS

μL	Microliter
μM	Micro molar
$^{\circ}\text{C}$	Degree celsius
cm	Centimeter
g	Gram
h	Hour
kV	Kilovolt
M	Molar (mol dm^{-3})
min	Minute
mm	Millimeter
mM	Millimolar
mL	Milliliter
mV	Millivolt
nm	Nanometer
R^2	Square of correlation coefficient
s	Second
U	Unit
V	Volt